



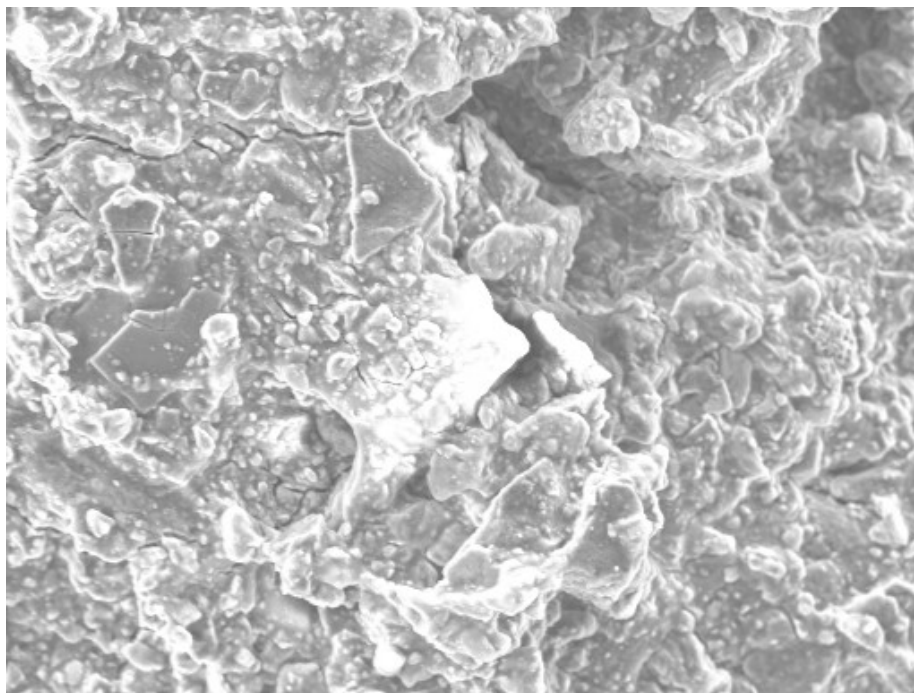

Title	: IMG1
Instrument	: JCM-6000PLUS
Volt	: 15.00 kV
Mag.	: x 300
Date	: 2022/02/20
Pixel	: 512 x 384

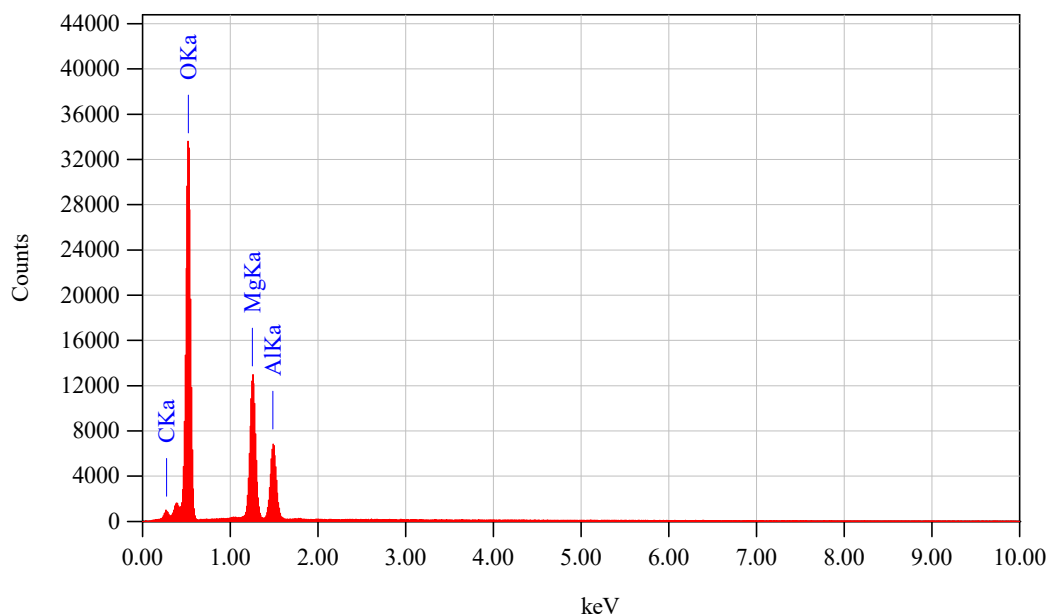

Acquisition Parameter	
Instrument	: JCM-6000PLUS
Acc. Voltage	: 15.0 kV
Probe Current	: 7.47500 nA
PHA mode	: T3
Real Time	: 55.23 sec
Live Time	: 50.00 sec
Dead Time	: 9 %
Counting Rate	: 10309 cps
Energy Range	: 0 - 20 keV

Thin Film Standardless Standardless Quantitative Analysis

Fitting Coefficient : 0.0153

Element	(keV)	Mass%	Counts	Sigma	Atom%	Compound	Mass%	Cation	K
C K*	0.277	2.69	3624.98	0.03	4.09				2.5867
O K* (Ref.)	0.525	61.03	212902.45	0.15	69.65				1.0000
Mg K*	1.253	22.95	106748.55	0.11	17.24				0.7498
Al K*	1.486	13.34	58881.78	0.09	9.02				0.7901
Total		100.00			100.00				